

CHARITY HOSPITAL  
STATE OF LOUISIANA  
NEW ORLEANS

Finger ring

Washer which fits over plunger  
and screws into ring cap thus  
fastening it into place.

Spring strip which increases plunger  
syringe friction by pressing on  
cap.


Screw cap

Thin brass tubing containing offset pieces  
containing screw threads for  
cap + valve piston.

Slider to adjust outward motion  
of plunger.

Brass tubing to contain four windows  
to permit visibility of syringe.

7 Parts to assemble

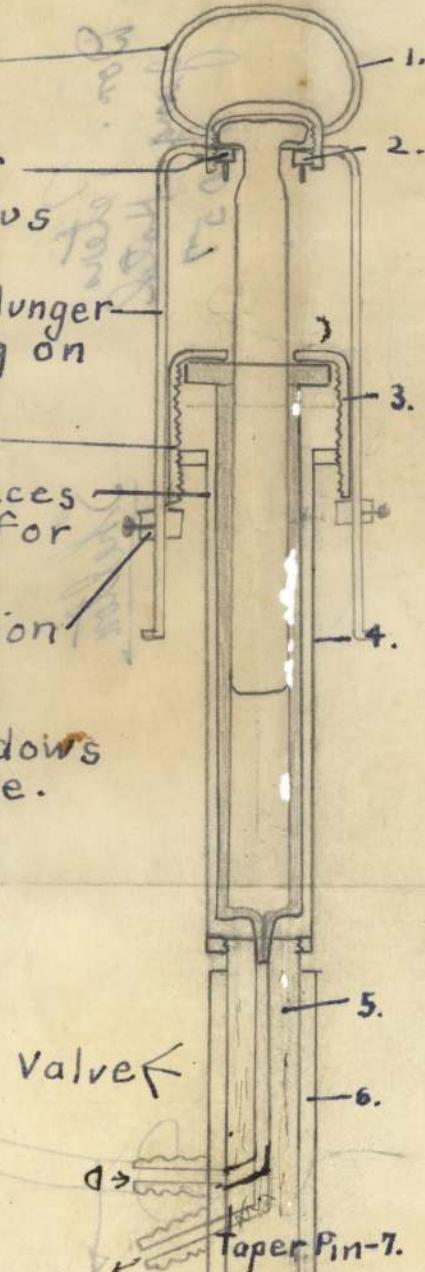


Improvements in the  
syringe case and friction  
adjusting mechanism & slider  
to limit outward motion of the  
piston.

6 x 2 x 1 1/2

CHARITY HOSPITAL  
STATE OF LOUISIANA  
NEW ORLEANS

Don. Peters  
Aug 10, 57  
Hotel

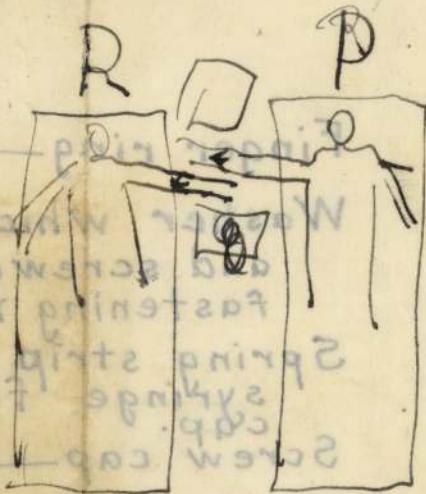

Brake cylinder piston pushes screw cap into frame.  
Frame is forced into cylinder piston.  
Screw cap is forced into frame.


Shelton

This pressurized piston is offset by counterbalanced eccentric piston to adjust cylinder to screw cap.

Allows cylinder to adjust automatically without  
to permit visibility of screw.

Parts to assemble

Valve

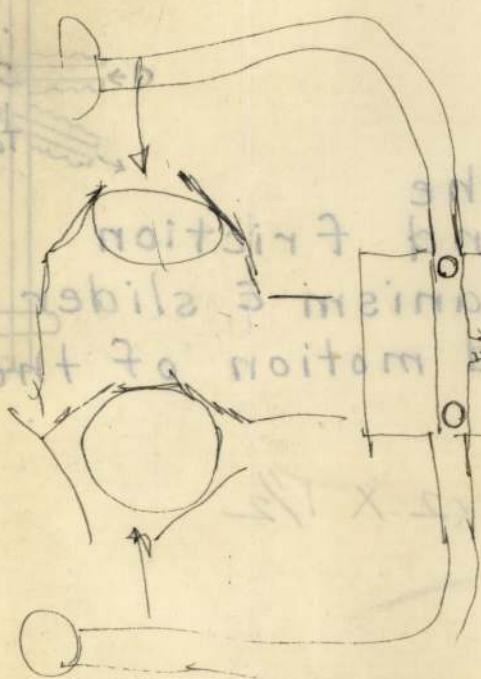

Implications in this  
cylinder case the  
adjusting mechanism  
is able to limit motion  
of piston.